


NeoNatalie Resuscitator Oxygen kit

User Guide

REF Cat.No. 846141 **QTY** 1 each

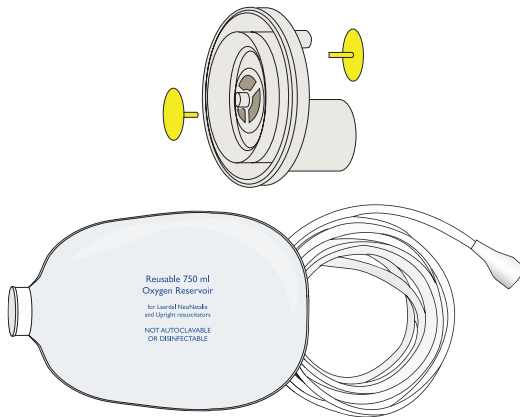



This oxygen kit is an accessory to the Laerdal NeoNatalie Resuscitator, Cat. No. 846040. The NeoNatalie Resuscitator's User Guide applies fully also when used with this NeoNatalie Resuscitator Oxygen kit User Guide.

1 Intended Use

The NeoNatalie Resuscitator with the Oxygen kit enables the delivery of oxygen-enriched air to the newborn. The oxygen kit may be reused provided proper cleaning and sterilization or disinfection procedures are performed between each patient use.

2 Items Included / Overview

- Directions for Use – Oxygen kit

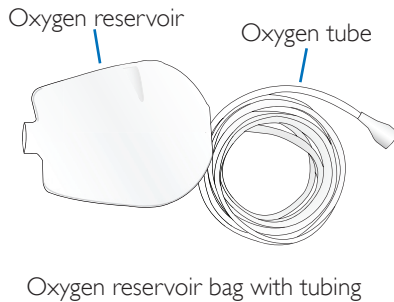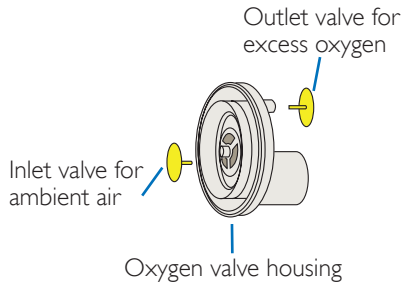

3-4

Not used.

5 Safety when using oxygen


1. Build-up and transfer of high pressure to the patient is prevented since excess O_2 is vented to atmosphere over the outlet membrane of the Intake Valve.
2. When O_2 supply is insufficient, adequate ventilation volume is ensured by intake of ambient air over the intake membrane of the Intake Valve.
3. In the presence of high oxygen concentrations there is danger from smoking or naked flames. Oil or grease must not be used with the resuscitator.
4. A Reservoir Bag that stays flat during the whole ventilation cycle is a visual indication that none, or little supplemental O_2 is being provided.

6 General Hygiene

Before first-time use, dis-assemble the oxygen kit and wash and clean as described for in Section 10.

7 Check Before Each Use



1. Attach the Oxygen valve housing onto the resuscitator's inlet valve.
2. Fill the Reservoir Bag with ambient air by holding the Reservoir Bag over the patient port connector pressing with your thumb on the reservoir bag connector. Ensure tight seal between the patient port



and Reservoir Bag. Compress the bag with your other hand several times to inflate the reservoir bag with ambient air.


3. Attach the filled Reservoir Bag to the Oxygen valve housing.
4. Compression of the Reservoir Bag and visual rise of the outlet Flap Valve confirms that the Reservoir Valve efficiently vents excessive gas to atmosphere.
5. Perform several compression-release cycles on the ventilation bag until the Reservoir Bag is flat and empty. Rapid re-expansion of the ventilation bag after flattening of the Reservoir Bag confirms that the Reservoir Valve efficiently lets in ambient air.

8 Using the Oxygen kit


- 
1. Screw the Oxygen valve housing onto the resuscitator's inlet valve.
 2. Attach the oxygen tube to the oxygen valve housing and the oxygen source, for higher oxygen concentrations.
 3. Attach the reservoir bag to the oxygen valve housing, for higher oxygen concentrations.
 4. See Section 14 for oxygen concentrations.
- 

9 Dis-assembling the Oxygen kit

Dis-assemble the resuscitator before performing the cleaning procedure.

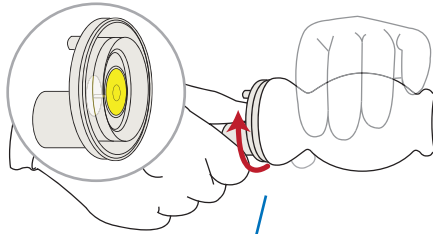

Unscrew the rear end of the intake valve housing from the bag.

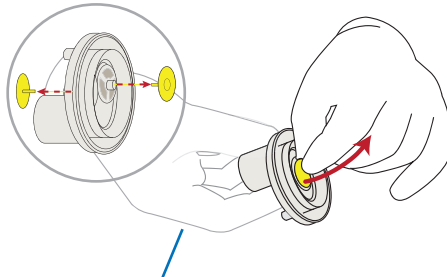

Remove both oxygen umbrella valves from the rear end of the intake valve housing.

10 Cleaning and Disinfection

After each use, dis-assemble and clean the oxygen kit parts:

- Wipe off the oxygen tube and oxygen reservoir with soapy water only on the outside surfaces. Rinse the outside surfaces in clean water.
- Wash and scrub the housing and valve parts in soapy water.
- Rinse in clean water.
- The oxygen valve parts may be sterilized by autoclaving or disinfected as described in the NeoNatalie Resuscitator User Guide.
- Visually inspect each part for damage and cleanliness / mineral deposits. Remove damaged or unclean parts from service. See NeoNatalie Resuscitator User Guide for descaling instructions..



Note: The Reservoir bag and tubing cannot be sterilized.



Warning: Discard Oxygen Reservoir Bag and Oxygen Tube if interior surfaces have been contaminated.

11 Re-assembling the Oxygen kit

To re-assemble the Oxygen kit, perform the steps described under Section 9 - in reverse.

12-13

No amendments. Refer to the NeoNatalie Resuscitator's User Guide.

14 Technical Information

Delivered oxygen concentration measured at approx. 23 °C:

	20 ml tidal volume 60 breaths/min		150 ml tidal volume 25 breaths/min	
Oxygen flow	Without reservoir bag	With reservoir bag	Without reservoir bag	With reservoir bag
2 LPM	52 %	71 %	56 %	84 %
4 LPM	60 %	97 %	58 %*	99 %**
6 LPM	58 %	98 %	60 %	94 %

* At -18 °C: 53%. At 50 °C: 47%

** At -18 °C: 66%. At 50 °C: 88%

Specifications

Materials:

- Reservoir bag and oxygen tube: Polyvinylchloride (PVC)
- Hard plastic components: Polysulfone (PSU)
- Valves: Silicones (SI)

Weight:

Approx. 80 grams

Dimensions:

Resuscitator with oxygen kit: Approx. 440 mm x 70 mm x 180 mm

CE 2460

This product is in compliance with the essential requirements of Council Directive 93/42/EEC as amended by Council Directive 2007/47/EC.

Global Warranty

See www.laerdal.com

Manufactured in China for:
Laerdal Medical AS, Tanke Svilandsgate 30
P.O. Box 377, 4002 Stavanger, Norway

Tel. +47 51 51 17 00.
Fax +47 51 52 35 57.

NeoNatalie Resuscitator; Newborn - Reusable, the Laerdal Logo, and "helping save lives" are all trademarks of Laerdal Medical.
© 2017 Laerdal Medical AS. All rights reserved.



Laerdal
helping save lives